

Development of an *in-situ* CO₂ gradient sampler



Laurin Osterholt, Martin Maier
Forest Research Institute Baden-Württemberg (FVA), Freiburg, Germany

01.05.2020


Introduction

Measuring soil gas flux with the gradient method

- in situ measurement
 - macrostructure is included
 - temporal variability can be monitored
- no disturbance of soil-atmosphere interface
- information about depth profile

but:


- diffusion coefficient (D_S) needed for flux calculation
 - injection of a tracer gas to calculate D_S inversely



Concept

Development of a sampler with built in CO₂ sensors

- construction with separate 3D-print segments
- flexible amount of depths
- continuous measurements in multiple depths
- identification of short term effects possible




Features

Inflatable gaskets between each measurement depth

→ prevent gas bypassing



Tracer gas injection at the bottom of the sampler



Installation



drill a hole

01.05.2020



insert sampler



inflate gaskets





inject tracer

Modelling of diffusion coefficient

CO₂ as tracer gas

- CO₂ can be measured with low cost sensors
→ no need for gas chromatography
- second reference sampler is used to measure respiration profile




Modelling of diffusion coefficient

CO₂ as tracer gas

- CO₂ can be measured with low cost sensors
→ no need for gas chromatography
- second reference sampler is used to measure respiration profile

tracer profile = injection profile - reference profile

$D_s = \text{injection rate} / \text{slope of tracer profile}$



Modelling of D_s with COMSOL

Finite Element modelling of D_s

Tracer injection experiment in sand- and gravel box

→ System without respiration



injection in gravel box

Modelling of D_s with COMSOL


Finite Element modelling of D_s

Tracer injection experiment in sand- and gravel box

→ System without respiration

2D axisymmetric modelling of CO_2 concentration with COMSOL¹

modelled CO_2 profile



¹COMSOL Multiphysics® v. 5.2a. www.comsol.com.
COMSOL AB, Stockholm, Sweden.

Modelling of D_s with COMSOL

Finite Element modelling of D_s


Tracer injection experiment in sand- and gravel box

→ System without respiration

2D axisymmetric modelling of CO_2 concentration with COMSOL¹

Optimizing D_s until modelled CO_2 fits measurements

Evaluation of the sampler still in progress

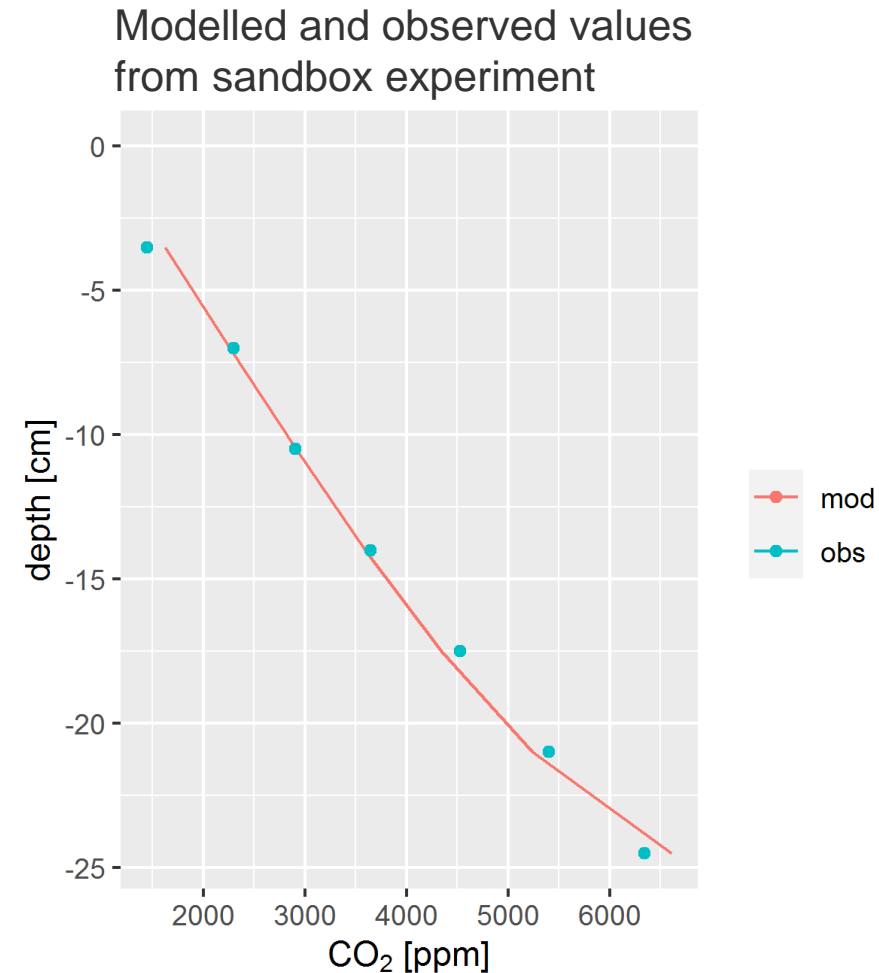

¹COMSOL Multiphysics® v. 5.2a. www.comsol.com.
COMSOL AB, Stockholm, Sweden.

Thanks for your attention!

Any questions?

I'll be there to answer them in the chat

8 may 10:45 – 12:30